

## ORIGINAL ARTICLE

# Influence of the layer thickness on the flexural strength of aged and nonaged additively manufactured interim dental material

Michael Scherer DMD, MS<sup>1,2</sup> | Nadin Al-Haj Husain DDS, MDM<sup>3,4</sup> |  
 Abdul B. Barmak MD, MSc, EdD<sup>5</sup> | John C. Kois DMD, MSD<sup>6,7,8</sup> |  
 Mutlu Özcan DDS, DMD, PhD<sup>9</sup> | Marta Revilla-León DDS, MSD, PhD<sup>6,7,10</sup>

<sup>1</sup>School of Dentistry, Loma Linda University, Loma Linda, CA

<sup>2</sup>Private Practice, Sonora, CA

<sup>3</sup>Division of Dental Biomaterials, Clinic for Reconstructive Dentistry, Center of Dental Medicine, University of Zurich, Zurich, Switzerland

<sup>4</sup>Department of Reconstructive Dentistry and Gerodontology, School of Dental Medicine, University of Bern, Bern, Switzerland

<sup>5</sup>Institute of Oral Health, University of Rochester Medical Center, Rochester, NY

<sup>6</sup>Kois Center, Seattle, WA

<sup>7</sup>Department of Restorative Dentistry, School of Dentistry, University of Washington, Seattle, WA

<sup>8</sup>Private Practice, Seattle, WA

<sup>9</sup>Division of Dental Biomaterials, Clinic for Reconstructive Dentistry, Center of Dental Medicine, University of Zürich, Switzerland

<sup>10</sup>Department of Prosthodontics, Tufts University, Boston, MA

## Correspondence

Dr. Marta Revilla-León, 1001 Fairview Ave N # 2200, Seattle, WA 98109.

Email: [marta.revilla.leon@gmail.com](mailto:marta.revilla.leon@gmail.com)

## Abstract

**Purpose:** To measure the flexural strength and Weibull characteristics of aged and nonaged printed interim dental material fabricated with different layer thickness.

**Material and methods:** Bars (25×2×2 mm) were additively fabricated by using a polymer printer (Asiga Max) and an interim resin (Nexdent C&B MFH). Specimens were fabricated with the same printing parameters and postprocessing procedures, but with 7 different layer thickness: 50 (control or 50-G group), 10 (10-G group), 25 (25-G group), 75 (75-G group), 100 (100-G group), 125 (125-G group), and 150 μm (150-G group). Two subgroups were created: nonaged and aged subgroups (n = 10). A universal testing machine was selected to measure flexural strength. Two-parameter Weibull distribution values were computed. Two-way ANOVA and Tukey tests were selected for statistical evaluation of the data ( $\alpha = 0.05$ ).

**Results:** Artificial aging methods ( $p < 0.001$ ) were a significant predictor of the flexural strength computed. Aged specimens acquired less flexural strength than nonaged specimens. The Weibull distribution obtained the highest shape for nonaged 50-G and 75-G group specimens compared with those of other nonaged groups, while the Weibull distribution showed the highest shape for aged 125-G specimens.

**Conclusions:** The flexural strength of the additively fabricated interim material examined was not influenced by the layer thickness at which the specimens were fabricated; however, artificial aging techniques reduced its flexural strength. Aged specimens presented lower Weibull distribution values compared with nonaged specimens, except for the 125-G specimens.

## KEYWORDS

3D printing, additive manufacturing technologies, interim dental prostheses, provisional dental material, vat-polymerization technologies

Digital light processing (DLP) procedures are considered vat-polymerization additive manufacturing (AM) techniques. DLP methods are clinically relevant methods to fabricate interim dental materials.<sup>1,2</sup> While the methods and manufacturing technologies used to fabricate them have been evaluated, the chemical composition, optimal printing and postprocessing parameters, and mechanical characteristics of vat-polymerized interim dental materials are still uncertain.<sup>3,4</sup>

The characteristics and physical properties of AM interim materials<sup>5–20</sup> including manufacturing accuracy,<sup>11,16</sup> chemical composition,<sup>9</sup> color,<sup>5,12</sup> surface roughness,<sup>9,11,14,20</sup>

marginal and internal fit,<sup>13,16,19</sup> mechanical properties,<sup>5,6,8,10,11,15,18</sup> adhesion of the microbiota,<sup>11</sup> wear,<sup>7</sup> and impact of accelerating aging techniques<sup>5,6,19,10</sup> have been analyzed in dental literature. An association has been recognized between the elected fabricating protocols (printing parameters and postprocessing methods) and the characteristics of the 3D printed devices including interim dental restoration.<sup>4</sup> Furthermore, there is a correlation among the additive technology, printer, and resin elected to process the dental device.<sup>4</sup> Dental literature has not been able yet to determine the optimal printing protocol based on the manufacturing trinomial, manufacturing protocol, and dental device.

Layer thickness has been recognized as one of the manufacturing variables that can affect the surface roughness, manufacturing accuracy, marginal and internal fit, fabricating time, and degree of conversion of 3D printed dental devices including interim dental restorations.<sup>3,13,14,17,21</sup> Furthermore, printed interim restorations exposed to aging techniques demonstrated lower flexural strength,<sup>5,6,10</sup> color stability,<sup>5</sup> and internal and marginal discrepancies<sup>19</sup> when compared to nonaged AM interim restorations. While many of the previously mentioned manufacturing variables have been evaluated in the scientific literature, the flexural strength and Weibull characteristics between aged and nonaged 3D printed interim materials fabricated with varying layer thickness remain unknown.

The goal of this investigation was to measure the flexural strength and Weibull characteristics of aged and nonaged AM interim dental material fabricated with varying layer thickness (10, 25, 50, 75, 100, 125, and 150  $\mu\text{m}$ ). The null hypotheses were that no significant discrepancy on the flexural strength and Weibull characteristics would be found among the specimens manufactured using different layer thicknesses and that no significant discrepancy on the flexural strength and Weibull characteristics would be found between aged and nonaged specimens.

## MATERIAL AND METHODS

A digital bar-shape (25 $\times$ 2 $\times$ 2 mm)<sup>22</sup> specimen was obtained by using a software program (Blender, version 2.77a; The Blender Foundation). All the manufacturing methods were accomplished by a prosthodontist (M.S.) with more than 10 years of preceding experience managing vat-polymerization printers.

The virtual bar-shape design was used to additively fabricate all the interim bars by using a polymer vat-polymerization printer (Asiga Max; Asiga) and a resin designated for interim restorations (Nexdent C&B MFH Shade N1; 3D Systems). The printer was stored in a room with constant temperature of 23°C and was calibrated according to the manufacturer's calibration procedure prior to producing any specimen. A fresh bottle of resin was obtained to manufacture all the specimens. Except for layer thickness, the bars of each group were processed all together with identical printing protocols, including same location in the build platform, print orientation, and supportive material (Fig 1). All the bars were positioned in the build platform so that the layer was perpendicular to the load to be applied in the fracture resistance test.

Seven groups were produced depending on the layer thickness chosen to fabricate the specimens: 10 (10-G group), 25 (25-G group), 50 (control or 50-G group), 75 (75-G group), 100 (100-G group), 125 (125-G group), and 150  $\mu\text{m}$  (150-G group). The 50-G group was treated as the control group because 50- $\mu\text{m}$  is the layer thickness endorsed by the manufacturer (Table 1).

After completing the manufacturing procedures, the post-processing rinsing and polymerization procedures were completed following the manufacturer's protocol. First, a spatula was used to remove the specimens from the build platform. Then, the specimens were washed in a 91% isopropyl alcohol (IPA) (Isopropyl alcohol 91%; Cumberland Swan) bath for 3 minutes, followed by a second 91% IPA clean bath for another 2 minutes. The specimens were dried on a paper towel and polymerization procedures were completed (LC-3DPrint Box; 3D Systems) at 300 to 550 nm for 30 minutes. Lastly, a removal tool was used to remove the supportive material. The bars were stored in a light-proof bottle until the tests were performed.

Twenty bars per group were obtained, and arbitrarily distributed into 2 subgroups by using a shuffled deck of cards depending on the artificial aging techniques: nonaged and aged subgroups (N = 20, n = 10). Sample size was established based on previous investigations.<sup>6</sup> In the aged subgroup, the bars were exposed to thermocycling methods which included 6000 cycles of 3 successive sequences each: (1) 20 seconds (dwelling phase) at 5°C; (2) 5 seconds (transfer phase) at ambient air temperature at 23°C; and (3) 20 seconds (dwelling phase) at 55°C.

A universal testing machine (Universal Testing Machine; ZwickRoell) at a crosshead speed of 1mm/min on a 10-mm span was elected to measure flexural strength (MPa).<sup>22</sup> The bars were loaded to failure and fracture load (N) data were documented. The flexural strength ( $\sigma$ ) was calculated using the formula:  $\sigma = 3 \times F_{\text{max}} \times L / 2 \times b \times d^2$ , where  $F_{\text{max}}$  is the failure load (force) at the fracture point (N), L is the length of the support span (10 mm), b is the width, and d is the thickness of the bar.<sup>17</sup>


Weibull distribution maximum likelihood estimation without a correction factor was used including the Weibull modulus, scale (m), and shape (0) to interpret the predictability and reliability of the flexural strength tests (Minitab Software V.16; Minitab).<sup>23</sup>

The Shapiro-Wilk and Kolmogorov-Smirnov tests disclosed that the data presented a normal distribution ( $p < 0.05$ ). Two-way ANOVA and post hoc multiple pairwise comparison Tukey tests were selected for statistical evaluation of the data ( $\alpha = 0.05$ ) (IBM SPSS Statistics for Windows, v26; IBM Corp).

## RESULTS

Two-way ANOVA indicated that only the accelerating artificial aging methods (df = 1, MS = 238829, F = 583.16, P < .001) was a significant predictor of the flexural strength measured (Fig 2a, Table 2). Additionally, the artificial aging technique explains the 80.33% difference in the flexural strength obtained, while the layer thicknesses evaluated explains the 1.49% disparity in the flexural strength computed.

With respect to the group factor, Tukey pairwise comparison revealed no significant flexural strength differences

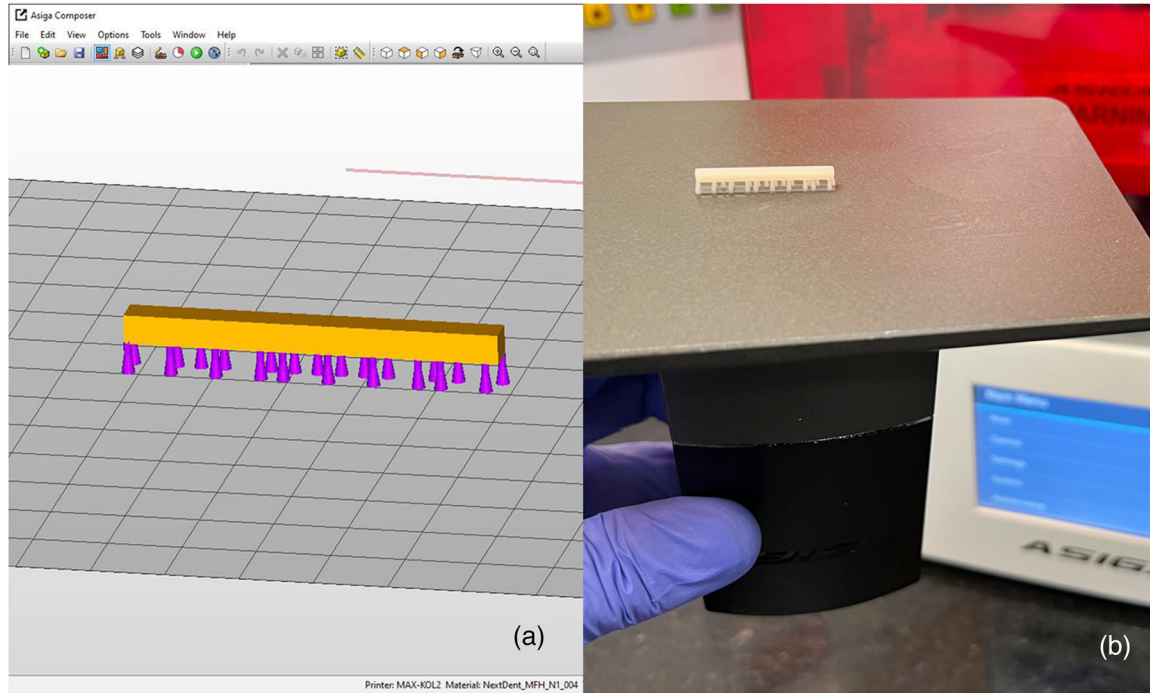

**FIGURE 1** (a) Representative specimen orientation. (b) Representative AM specimen. AM, additively manufactured.

**TABLE 1** Characteristics of the groups assessed

Group	Subgroup	Layer thickness	Aging methods
10-G	Aged	10 $\mu\text{m}$	Yes
	Nonaged		No
25-G	Aged	25 $\mu\text{m}$	Yes
	Nonaged		No
50-G	Aged	50 $\mu\text{m}$	Yes
	Nonaged		No
75-G	Aged	75 $\mu\text{m}$	Yes
	Nonaged		No
100-G	Aged	100 $\mu\text{m}$	Yes
	Nonaged		No
125-G	Aged	125 $\mu\text{m}$	Yes
	Nonaged		No
150-G	Aged	150 $\mu\text{m}$	Yes
	Nonaged		No

among the differing layer thicknesses tested. With respect to the subgroup predictor, Tukey pairwise comparison demonstrated significant flexural strength discrepancies between nonaged (mean of 289.77 MPa) and aged specimens (mean of 207.17 MPa) (Fig 2b).


The Weibull distribution obtained the highest shape for nonaged 50-G (control) (45.98) and 75-G group specimens (42.24) compared with those of other nonaged groups (11.36-27.12), while the Weibull distribution showed the highest

shape for aged 125-G specimens (68.18) compared with those of other aged groups (10.62-44.58) (Fig 3).

## DISCUSSION

The results of this investigation demonstrated that the specimens fabricated with different layer thicknesses using the polymer vat-polymerization DLP 3D printer tested, with its specific manufacturing protocol described, obtained no significant discrepancies in the flexural strength computed. But accelerating artificial aging techniques caused in a significant reduction in the flexural strength mean values of the 3D printed interim material tested. Hence, only the second null hypothesis was rejected.

The differing layer thicknesses assessed on the specimens manufactured using the selected interim dental resin, DLP printer, and manufacturing protocol tested on this investigation did not significantly influence the flexural strength values obtained. Therefore, just considering the flexural strength characteristics, interim dental restorations could be manufactured using any of the layer thicknesses tested. However, dental literature has shown a correlation between layer thickness, surface roughness, manufacturing accuracy, fabricating time, and degree of conversion of AM dental devices.<sup>13,14,17,21</sup> Additionally, the generalization of the results is not recommended as the characteristics of the printed device are the result of multiple manufacturing variables such as technology, printer, and resin chosen, printing parameters, or postprocessing processes performed. Therefore, additional studies might be needed to assess the influence of the layer thickness on the mechanical properties

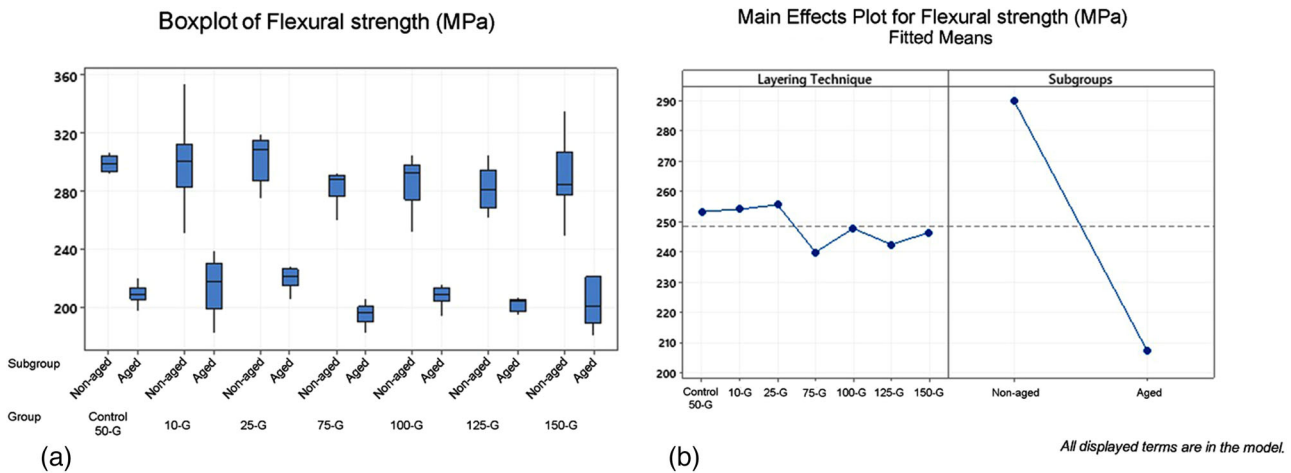

**FIGURE 2** (a) Boxplot of flexural strength values obtained among the groups. (b) Main effects plot for flexural strength obtained among the groups.

**TABLE 2** Flexural strength values (MPa) obtained among the groups tested

Group	Subgroup	Flexural strength mean $\pm$ SD values (MPa)
50-G	Nonaged	296.6 $\pm$ 11.97
	Aged	210.1 $\pm$ 6.69
10-G	Nonaged	298.9 $\pm$ 28.70
	Aged	209.3 $\pm$ 33.01
25-G	Nonaged	290.5 $\pm$ 46.01
	Aged	220.7 $\pm$ 6.98
75-G	Nonaged	283.6 $\pm$ 10.33
	Aged	196.0 $\pm$ 7.33
100-G	Nonaged	286.6 $\pm$ 17.29
	Aged	208.9 $\pm$ 6.61
125-G	Nonaged	282.0 $\pm$ 15.30
	Aged	202.8 $\pm$ 4.16
150-G	Nonaged	290.2 $\pm$ 24.21
	Aged	202.5 $\pm$ 14.91

SD, standard deviation.

of varying 3D printed devices before further conclusions can be done.

Different manufacturing variables can affect the characteristics of AM interim specimens.<sup>5–21</sup> To limit these factors, the specimens were fabricated from a single bottle of dental resin with the same printing parameters (except for the layer thickness), location in the build platform, and postprocessing methods. Furthermore, the bar-shape specimens were fabricated following the ISO recommended dimensions<sup>22</sup> with the layer orientation positioned perpendicular to the load direction of the 3-point bend test to optimize the flexural strength of the printed interim material.<sup>15</sup> However, in the present study, the printer and the material tested were not from the same manufacturer. The material manufacturer offers a vat-polymerization printer; however, the layer

thickness could not be modified as it is a closed system. Therefore, an open printer was selected to assess the influence of the material layer thickness on the flexural strength and Weibull characteristics.

Limited studies have tested the flexural strength of interim materials processed using AM technologies.<sup>5,6</sup> Scotti et al<sup>5</sup> reported a flexural strength value of  $105.10 \pm 9.80$  MPa for the same interim material tested (Nexdent C&B MHF). However, the specimens had different dimensions ( $10 \times 0 \times 2$  mm) and no details were provided regarding the printer, printing parameters, or postprocessing techniques selected to manufacture the specimens. Hence, comparisons with the data obtained in this investigation are difficult.

Scherer et al<sup>6</sup> assessed the influence of different postpolymerization times (25, 30, 35, 40, and 45 minutes) and conditions (dry, or inside a container containing water or glycerin) on the flexural strength of aged and nonaged bar-shape ( $25 \times 2 \times 2$  mm).<sup>22</sup> The specimens were fabricated using a resin designated to fabricate interim restorations (Nexdent C&B MHF) and a polymer printer (Nexdent 5100; 3D Systems). In the present investigation, the same resin was used, but a different polymer printer was elected (Asiga Max; Asiga). Variations in the printing or supportive parameters can be expected between both studies; however, further interpretation of how these discrepancies might impact the outcome of the printed specimens is unknown. Additionally, the postpolymerization methods were completed in dry conditions and performed for 30 minutes; thus, the results of the present investigation could be compared with the 30-minute and dry-condition postpolymerization groups. Scherer et al<sup>6</sup> reported a mean flexural strength value of  $274.85 \pm 15.64$  MPa for nonaged samples and  $267.84 \pm 34.34$  MPa for aged samples. Those results agree with the data obtained in this investigation.

Additional dental literature has evaluated the properties of printed interim restorations;<sup>8,24</sup> however, variations on the research methodology such as crown-shape specimens, fabrication protocols, and testing procedures make comparisons with the data obtained in this investigation challenging.

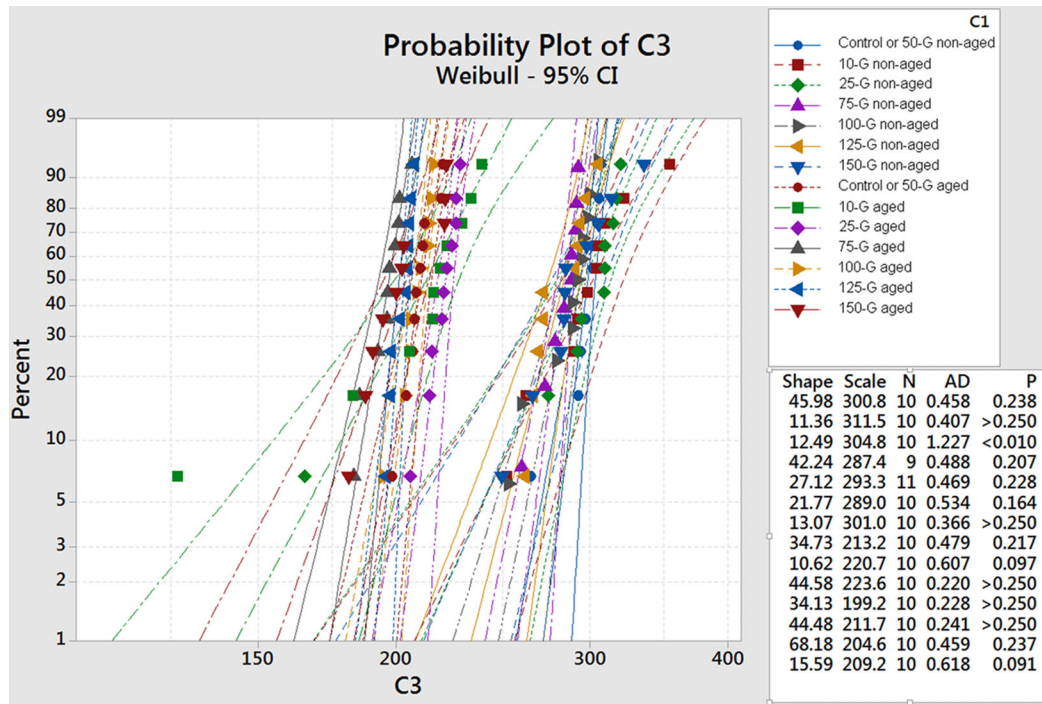


FIGURE 3 Weibull modulus for all the groups tested.

Thermal cycling techniques aim to reproduce the deterioration of the material in the oral environment.<sup>25</sup> The flexural strength of AM interim materials seems to be affected by artificial aging procedures.<sup>5,6,10</sup> The results of this investigation obtained a significant difference between nonaged (mean of 289.77 MPa) and aged specimens (mean of 207.17 MPa). While the phenomenon is multifactor, water absorption and matrix degradation of the resin is the suggested cause for this finding.<sup>26,27</sup> However, all the bars tested achieved a clinically acceptable flexural strength.<sup>28</sup>

Artificial intelligence (AI) models have been reported for optimizing manufacturing procedures.<sup>29,30</sup> This might be a tool in the future for establishing printing protocols based on the manufacturing trinomial and clinical application of the printed dental device. While the broad availability of printers and materials provide wider manufacturing options for dental professionals, there is a need for scientific literature that assesses the properties of these new materials, as well as, establishing optimal manufacturing protocols.

This investigation has limitations such as reduced additive technologies, 3D printers, and materials examined. Studies are suggested to further assess the influence of the different printing parameters on the fabrication accuracy, marginal and internal discrepancies, and physical characteristics of printed interim dental restorations.

CONCLUSIONS

Within the limitations of this in vitro investigation, the varying layer thickness tested did not affect the flexural strength

and Weibull characteristics of the interim material selected manufactured with the described DLP printer and printing protocol. However, artificial aging techniques reduced the flexural strength of the printed interim material assessed. Additionally, the Weibull distribution of flexural strength values on aged specimens were lower than those on nonaged specimens, with the exception of the 125-G specimens.

CONFLICT OF INTEREST

The authors did not have any conflict of interest, financial or personal, in any of the materials described in this study.

FUNDING

This research did not receive any specific grant from funding agencies in the public, commercial, or not-for-profit sectors.

REFERENCES

1. Revilla-León M, Özcan M. Additive manufacturing technologies used for processing polymers: current status and potential application in prosthetic dentistry. *J Prosthodont*. 2019;28:146–58.
2. Horn TJ, Harrysson OLA. Overview of current additive manufacturing technologies and selected applications. *Sci Prog*. 2012;95:255–82.
3. Revilla-León M, Meyers MJ, Zandinejad A, Özcan M. A review on chemical composition, mechanical properties, and manufacturing work flow of additively manufactured current polymers for interim dental restorations. *J Esthet Restor Dent*. 2019;31:51–7.
4. Piedra-Cascón W, Krishnamurthy VR, Att W, Revilla-León M. 3D printing parameters, supporting structures, slicing, and post-processing procedures of vat-polymerization additive manufacturing technologies: a narrative review. *J Dent*. 2021;109:103630.
5. Scotti CK, Velo MMDeAC, Rizzante FAP, Nascimento TRDeL, Mondelli RFL, Bombonatti JFS. Physical and surface properties of a

- 3D-printed composite resin for a digital workflow. *J Prosthet Dent.* 2020;124:614.e1–e5.
6. Scherer MD, Barmak AB, Özcan M, Revilla-León M. Influence of post-polymerization methods and artificial aging procedures on the fracture resistance and flexural strength of a vat-polymerized interim dental material. *J Prosthet Dent.* 2021; <https://doi.org/10.1016/j.prosdent.2021.02.017>
  7. Myagmar G, Lee J-H, Ahn J-S, Yeo In-SL, Yoon H-In, Han J-S. Wear of 3D printed and CAD/CAM milled interim resin materials after chewing simulation. *J Adv Prosthodont.* 2021;13:144–51.
  8. Martín-Ortega N, Sallorenzo A, Casajús J, Cervera A, Revilla-León M, Gómez-Polo M. Fracture resistance of additive manufactured and milled implant-supported interim crowns. *J Prosthet Dent.* 2022;127:267–74.
  9. Revilla-León M, Morillo JA, Att W, Özcan M. Chemical composition, knoop hardness, surface roughness, and adhesion aspects of additively manufactured dental interim materials. *J Prosthodont.* 2021;30:698–705.
  10. Reymus M, Fabritius R, Keßler A, Hickel R, Edelhoff D, Stawarczyk B. Fracture load of 3D-printed fixed dental prostheses compared with milled and conventionally fabricated ones: the impact of resin material, build direction, post-curing, and artificial aging—a *in vitro* study. *Clin Oral Investig.* 2020;24:701–10.
  11. Shim JS, Kim J-E, Jeong SH, Choi YJ, Ryu JJ. Printing accuracy, mechanical properties, surface characteristics, and microbial adhesion of 3D-printed resins with various printing orientations. *J Prosthet Dent.* 2020;124:468–75.
  12. Revilla-León M, Umorin M, Özcan M, Piedra-Cascón W. Color dimensions of additive manufactured interim restorative dental material. *J Prosthet Dent.* 2020;123:754–60.
  13. Park G-S, Kim S-K, Heo S-J, Koak J-Y, Seo D-G. Effects of printing parameters on the fit of implant-supported 3d printing resin prosthetics. *Materials (Basel).* 2019;12:2533.
  14. Arnold C, Monsees D, Hey J, Schweyen R. Surface quality of 3D-printed models as a function of various printing parameters. *Materials (Basel).* 2019;12:1970.
  15. Alharbi N, Osman R, Wismeijer D. Effects of build direction on the mechanical properties of 3D-printed complete coverage interim dental restorations. *J Prosthet Dent.* 2016;115:760–7.
  16. Alharbi N, Osman R, Wismeijer D. Factors influencing the dimensional accuracy of 3d-printed full-coverage dental restorations using stereolithography technology. *Int J Prosthodont.* 2016;29:503–10.
  17. Favero CS, English JD, Cozad BE, Wirthlin JO, Short MM, Kasper FK. Effect of print layer height and printer type on the accuracy of 3-dimensional printed orthodontic models. *Am J Orthod Dentofacial Orthop.* 2017;152:557–65.
  18. Tahayeri A, Morgan M, Fugolin AP, Bompolaki D, Athirasala A, Pfeifer CS, et al. 3D printed versus conventionally cured provisional crown and bridge dental materials. *Dent Mater.* 2018;34:192–200.
  19. Angwarawong T, Reeponmaha T, Angwaravong O. Influence of thermomechanical aging on marginal gap of CAD-CAM and conventional interim restorations. *J Prosthet Dent.* 2020;124:566.e1–e6.
  20. Revilla-León M, Jordan D, Methani MM, Piedra-Cascón W, Özcan M, Zandinejad A. Influence of printing angulation on the surface roughness of additive manufactured clear silicone indices: An *in vitro* study. *J Prosthet Dent.* 2021;125:462–8.
  21. Reymus M, Lümkeemann N, Stawarczyk B. 3D-printed material for temporary restorations: impact of print layer thickness and post-curing method on degree of conversion. *Int J Comput Dent.* 2019;22:231–7.
  22. International Organization for Standardization. ISO 10477:2018 Dentistry - Polymer-based crown and veneering materials. <https://www.iso.org/standard/68235.html>. Accessed 06/01/2019.
  23. Scherer MD, Al-Haj Husain N, Barmak AB, Kois JC, Özcan M, Revilla-León M. Influence of postprocessing rinsing solutions and duration on flexural strength of aged and nonaged additively manufactured interim dental material. *J Prosthet Dent.* 2022; <https://doi.org/10.1016/j.prosdent.2022.03.034>
  24. Quinn JB, Quinn GD. A practical and systematic review of Weibull statistics for reporting strengths of dental materials. *Dent Mater.* 2010;26:135–47.
  25. Park SM, Park JM, Kim SK. Comparison of flexural strength of three-dimensional printed three-unit provisional fixed dental prostheses according to build directions. *J Korean Dent Sci.* 2019;12:13–9.
  26. Gale MS, Darvell BW. Thermal cycling procedures for laboratory testing of dental restorations. *J Dent.* 1999;27:89–99.
  27. Topcu FT, Sahinkesen G, Yamanel K. Influence of different drinks on the colour stability of dental resin composites. *Eur J Dent.* 2009;3:50–6.
  28. ANSI/ADA Specification No. 27: Direct filling resins. American National Standards Institute, American Dental Association; Revised 1993.
  29. Revilla-León M, Gómez-Polo M, Vyas S, Barmak AB, Gallucci GO, Att W, et al. Artificial intelligence models for tooth-supported fixed and removable prosthodontics: a systematic review. *J Prosthet Dent.* 2021 [Epub ahead of print].
  30. Matin I, Hadzistevec M, Vukelic D, Potran M, Brajlilh T, et al. Development of an expert system for the simulation model for casting metal substructure of a metal-ceramic crown design. *Comput Methods Programs Biomed.* 2017;146:27–35.

**How to cite this article:** Scherer M, Al-Haj Husain N, Barmak AB, Kois JC, Özcan M, Revilla-León M. Influence of the layer thickness on the flexural strength of aged and nonaged additively manufactured interim dental material. *J Prosthodont.* 2022;1–6. <https://doi.org/10.1111/jopr.13582>